


ROUGH IN
Installation Drawing #1 - Cleo GX

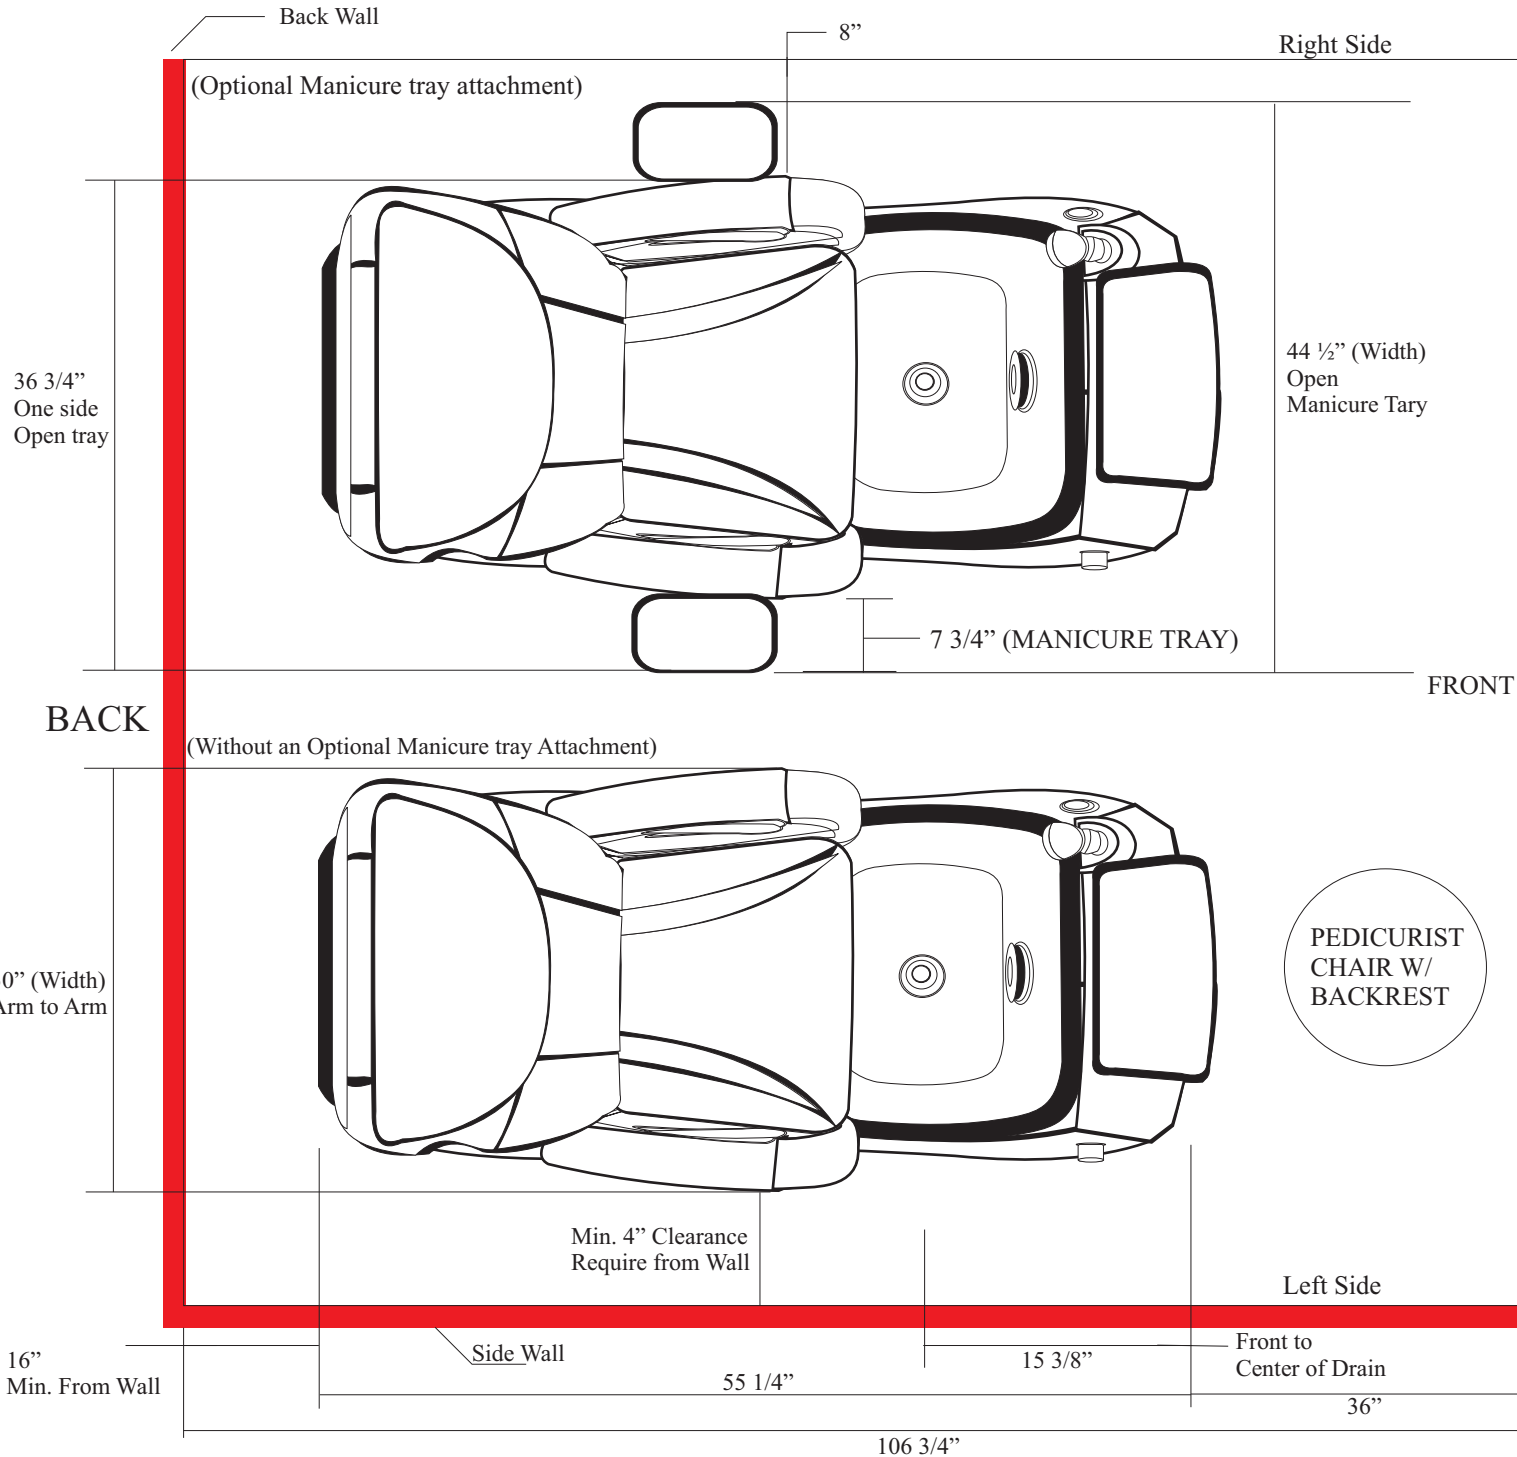

CAUTION - IMPORTANT

THIS DRAWING IS **NOT** COMPLETE UNLESS ACCOMPANIED BY PAGE 1 OF 2 ENTITLED: "INSTALLATION AND ROUGH IN INFORMATION"

PLEASE REVIEW ALL INFORMATION CAREFULLY.

VERY IMPORTANT

DEPENDING ON USE OF MANICURE TRAYS AND/OR CARTS, THE DISTANCE BETWEEN PEDICURE CHAIRS CAN VARY. THIS MUST BE DISCUSSED PRIOR TO INSTALLATION IN ORDER TO ENSURE ADEQUATE WORKING

ELECTRICAL REQUIREMENTS:

ONE DEDICATED GFGI PROTECTED WALL OUTLET (15 Amp.) **MUST** BE USED PER EACH UNIT.

PEDICURIST
CHAIR W/
BACKREST

LEGEND: DIMENSIONS ARE IN INCHES

Manufactured by :	Model :
J&A USA Inc.,	Cleo GX
Website	Prepared by :
www.jausainc.com	J&A USA Inc.

INSTALLATION DRAWING #2

Plumbing Rough - In (Back Wall Application)

Page 2 of 2


CAUTION - IMPORTANT

THIS DRAWING IS NOT COMPLETE UNLESS ACCOMPANIED BY PAGE 1 OF 2 ENTITLED: "INSTALLATION AND ROUGH IN INFORMATION"

PLEASE REVIEW ALL INFORMATION CAREFULLY.

VERY IMPORTANT

DEPENDING ON USE OF MANICURE TRAYS AND/OR CARTS, THE DISTANCE BETWEEN PEDICURE CHAIRS CAN VARY. THIS MUST BE DISCUSSED PRIOR TO INSTALLATION IN ORDER TO ENSURE ADEQUATE WORKING SPACE.

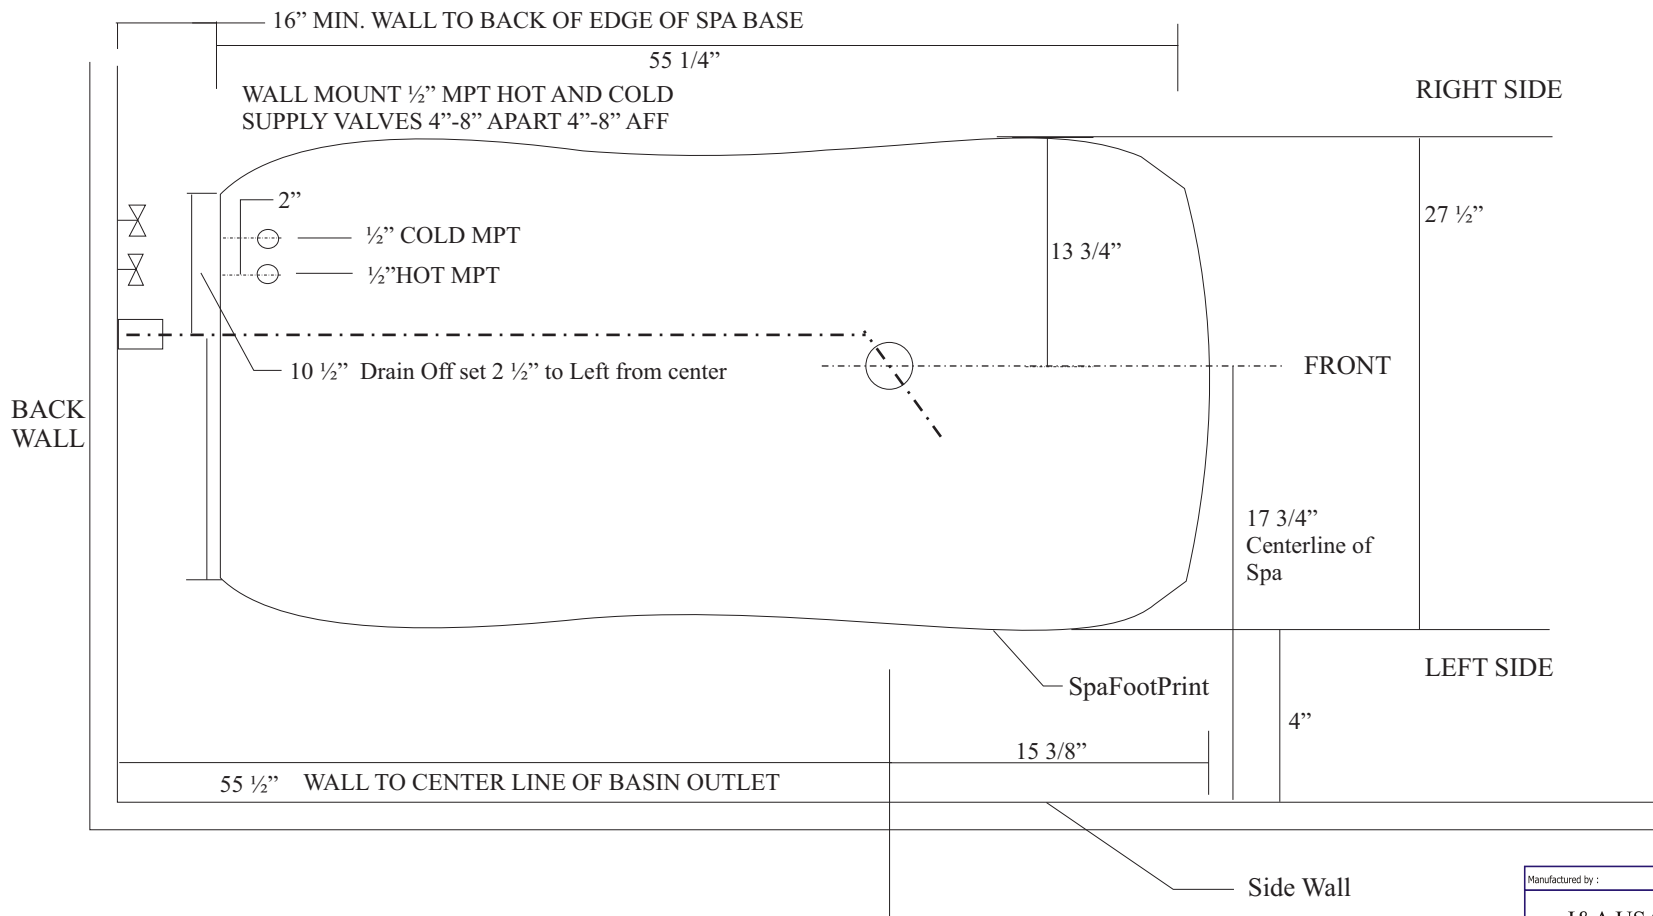

LEGEND:
ALL DIMENSIONS ARE IN INCHES

Manufactured by :	Model :
J&A USA Inc.,	Cleo GX
Website	Prepared by :
www.jausainc.com	J&A USA Inc.